


EPA Method 25.1 Assembly




Attach the bracket and cup to the SUMMA canister.



Attach the flow regulator and trap assembly. Regulator standard flow rate is 1 hour. Fill cup with dry ice.



2 micron stainless steel frit is installed at the probe end.

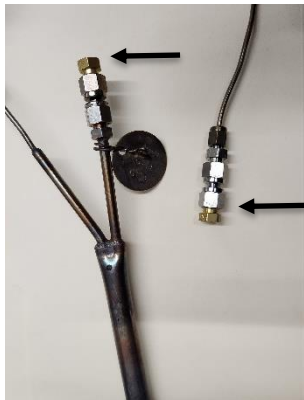

Cap both ends of the trap after sampling.

Place the traps in a cooler with dry ice for transport back to AtmAA laboratory.

AtmAA 818-223-3277